

# Editing Workspaces



In the DTS software, workspaces can be edited to user specifications by first selecting the workspace to be edited in the drop down list box, and then clicking the Configure button to the right of the list box (Figure 1). Within the Summary window, the type of measurements to be displayed, the parameters to be displayed in the Records View, and the Report pages to be displayed as tabs below the tool bar can be defined.

To add/remove parameters from the Record view, select the desired parameter and then use the arrow buttons to move the parameter. Note that you can edit the label of a parameter listed on the right hand side by double clicking the label cell. You should also be aware that some parameters require identifying values, e.g. the Size Peak parameter requires that you define the transform (intensity, volume, or number), the peak type (width, mean, area, or mode), and the peak number.


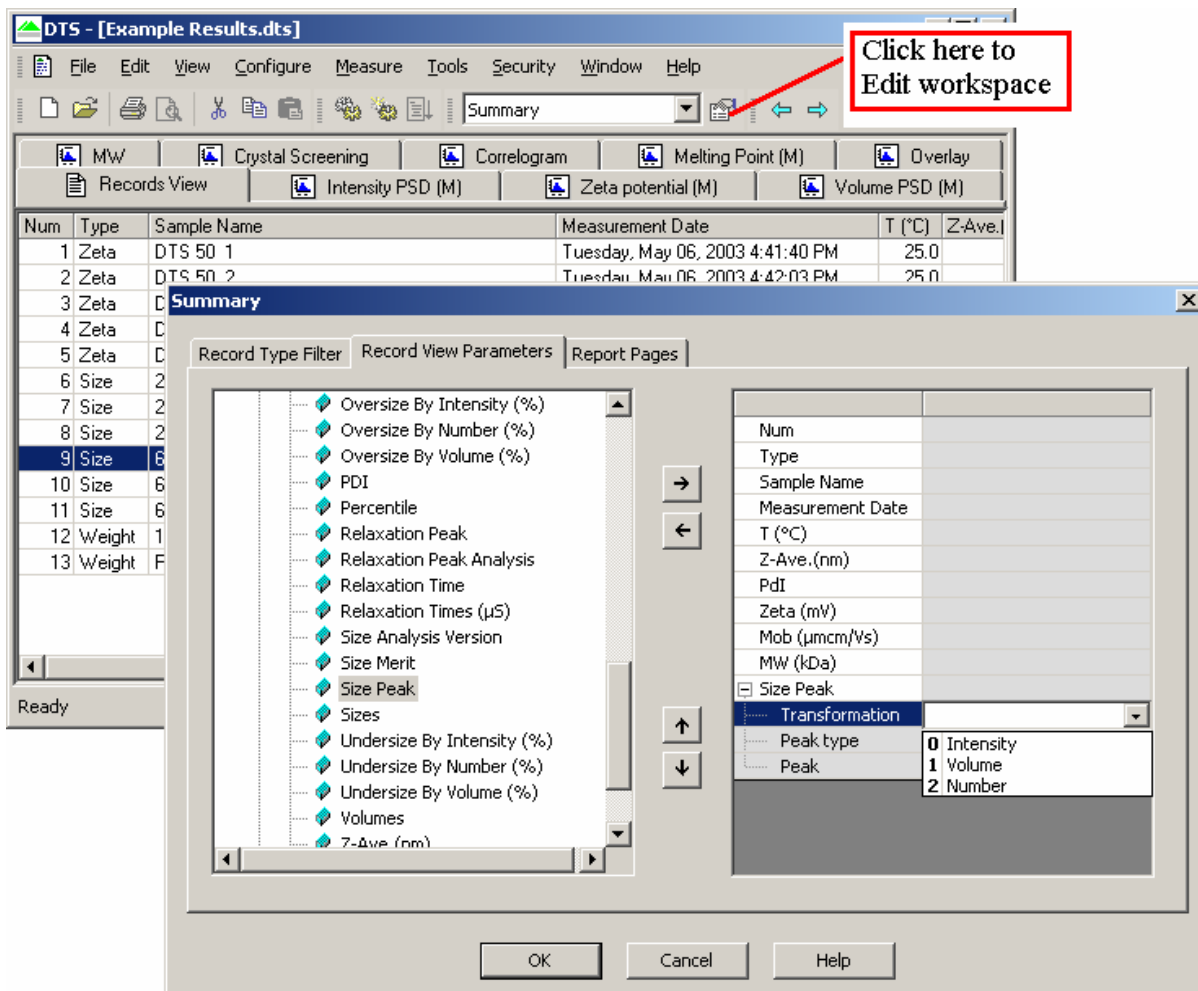


Figure 1: Editing workspaces to user specifications in the DTS software.

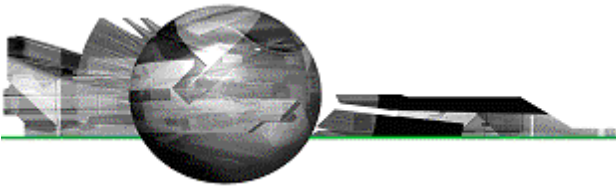

To add Report pages, select the Report Pages tab and the check the boxes of the reports you'd like to have available for that workspace. Custom reports can be created using the Report Designer option under the Tools option on the tool bar. Some advice on designing reports: it's much easier to start with an existing report, save it as a different name, and then edit it to suit your preferences.

**Malvern Instruments Ltd**

Enigma Business Park • Grovewood Road • Malvern • Worcestershire • UK • WR14 1XZ  
Tel: +44 (0)1684 892456 • Fax: +44 (0)1684 892789

**Malvern Instruments Worldwide**

Sales and service centers in over 50 countries for details visit [www.malvern.com/contact](http://www.malvern.com/contact)

[more information at www.malvern.com](http://www.malvern.com)